



Estrous Detector EDS2

data sheet

ANIMAL NUMBER

	date	hour	result
1			
2			
3			
4			
5			
6			
7			
8			
9			
10			
11			
12			
13			
14			
15			
16			
17			
18			
19			
20			

	date	hour	result
21			
22			
23			
24			
25			
26			
27			
28			
29			
30			
31			
32			
33			
34			
35			
36			
37			
38			
39			
40			

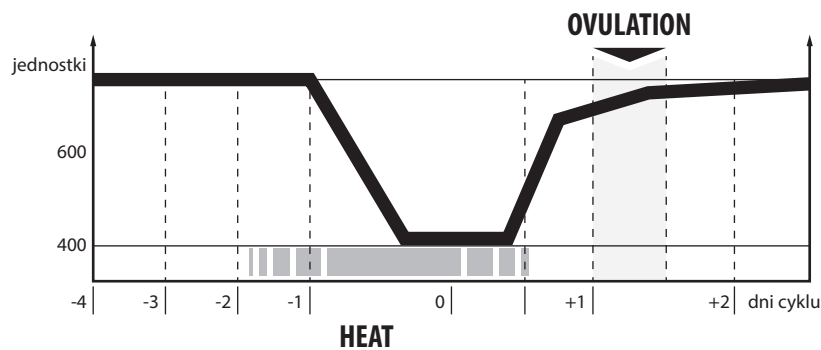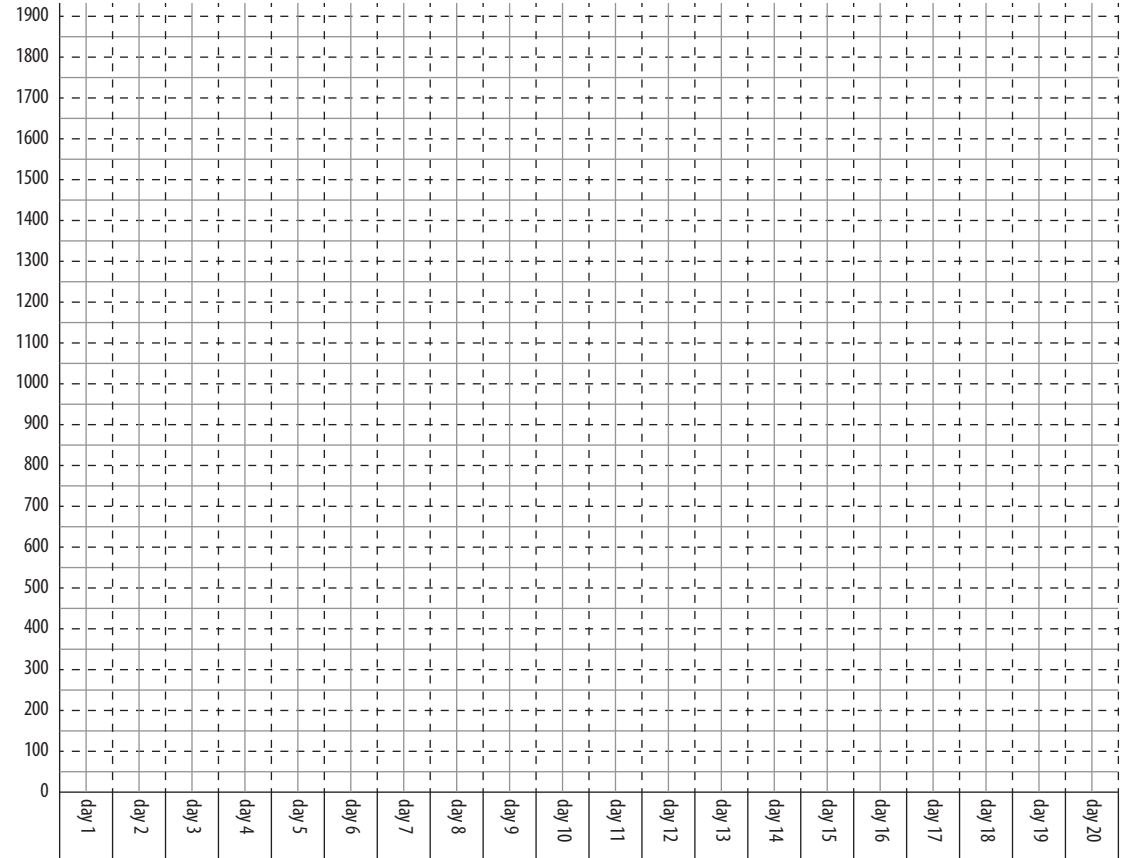

Sample graph of vaginal mucus resistance in sheep

Remember to:

- disinfect the probe
- remove the residual urine or other dirt from the vulva
- perform measurements always at the same depth
- rotate the probe inside the vagina before pressing the button
- perform measurements on a regular basis

**Always remember about
the hygiene and disinfection
of the probe
before and after each use**